

**COMPARISON OF METHODS FOR DETERMINATION OF HANDWEAR INSULATION
WITH A BIOPHYSICAL MODEL**

W. R. Santee and S. Kw. Chang
U.S. Army Research Institute of Environmental Medicine
Natick, Massachusetts, USA

INTRODUCTION

The conventional use of biophysical hand models has been to measure dry insulation from area weighted power demand values (1,2). This report describes two alternate methods for measuring dry insulation. One method is to determine the combined heat transfer coefficient for convection and radiation from the slope between power demand and multiple temperature differences. The second method consists of determining the total cooling rate of the model. The latter method is of interest because it is analogous to complete blockage of blood flow to the human hand as would occur with a severe wound, application of a tourniquet, total peripheral vasoconstriction or blood shunting. The analogy is not wholly complete because the specific heat coefficients (c_p) and masses of the model and a human hand are not equal.

METHOD

A seven section, water resistant aluminum hand model was used to calculate total thermal insulation by determining the change in cooling rate and by measuring power demand while maintaining constant surface temperatures. Insulation is calculated from the slope of power versus the difference between surface and air temperature. Cooling curves for both bare and covered models were generated by heating the model to a selected surface temperature setpoint (30°C), then cutting off the power supply. In this case, insulation is estimated from the relationship between the rate of temperature decline versus time. Power consumption versus temperature difference slope values were generated by measuring the sectional power consumption required to maintain a 30°C surface setpoint at different test chamber temperatures. Insulation values obtained with a 22-zone copper hand model were used as reference control values. Cooling curves were evaluated by calculating the slope for the natural logarithm of the temperature difference between the model surface temperature and the test chamber over time. Molnar (2) presents a similar calculation method.

TABLE 1. RESISTANCE AND INSULATION (CLO) VALUES FOR ISSUE MILITARY HANDWEAR

Table Ia. Comparison of two calculation methods and control values

	<u>control</u>	<u>weighted average</u> [*]	<u>slope</u>
	$m^2 \cdot K \cdot W^{-1}$ (clo)	$m^2 \cdot K \cdot W^{-1}$ (clo)	$m^2 \cdot K \cdot W^{-1}$ (clo)
bare hand	0.06 (0.4)	0.04 (0.2)	0.05 (0.3)
arctic mitten set	0.38 (2.4)	0.35 (2.2)	0.35 (2.3)
three finger mitten	0.23 (1.5)	0.21 (1.3)	0.21 (1.4)
light duty glove	0.14 (0.9)	0.12 (0.8)	0.12 (0.8)

Table Ib. Comparison of adjusted insulation values to control

	<u>control</u>	<u>weighted average</u> [*]	<u>slope</u>
	$m^2 \cdot K \cdot W^{-1}$ (clo)	$m^2 \cdot K \cdot W^{-1}$ (clo)	$m^2 \cdot K \cdot W^{-1}$ (clo)
bare hand	0.06 (0.4)	0.05 (0.3)	0.05 (0.3)
arctic mitten set	0.38 (2.4)	0.38 (2.5)	0.39 (2.5)
three finger mitten	0.23 (1.5)	0.23 (1.5)	0.23 (1.5)
light duty glove	0.14 (0.9)	0.14 (0.9)	0.13 (0.8)

^{*}mean of three repetitions, three values per repetition

FIGURE 1

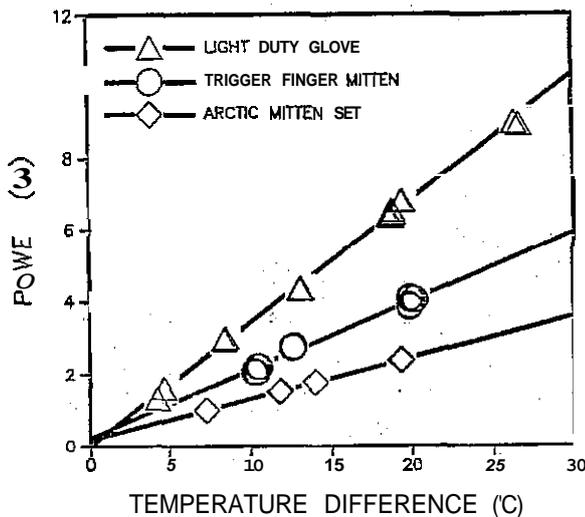


FIGURE 2

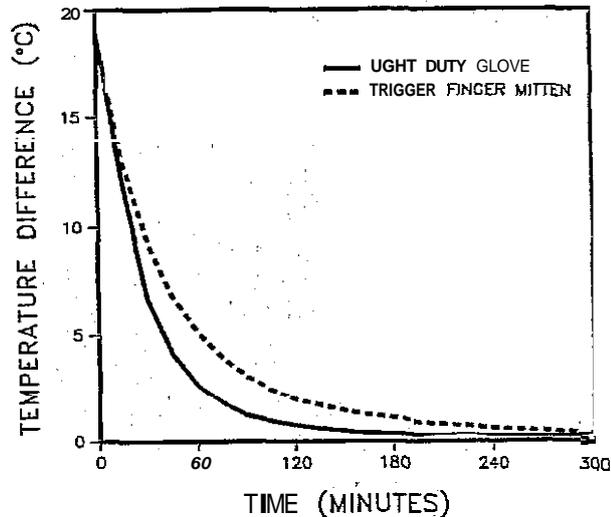


Figure 1. Power demand vs. temperature difference (ΔT) Figure 2. Temperature difference (ΔT) vs. time

RESULTS

Total insulation values (I_T) were calculated for current issue military handwear using both the area weighted power demand and slope methods (Table 1a). The insulation values for the new hand calculated by either method were 0.01-0.02 $m^2 \cdot K \cdot W^{-1}$ less than the control values obtained with the original copper hand model. Values calculated by the slope method were closer to the control values, but values were lower for both methods. When values were recalculated using a 10% larger total surface area to compensate for gaps between model sections, agreement with the control values increased (Table 1b). The relationship between power and the temperature difference is linear, whereas the relationship between surface temperature and time is curvilinear (Figures 1,2). The data obtained by cooling down the insulated hand model did not provide comparable calculated values for insulation, but relative levels of insulation of different handwear are indicated.

CONCLUSIONS

The power gradient slope method demonstrates an alternative method for calculating total handwear insulation (I_T) from power demand, and indicates that the values are constant over a range of temperature gradients. However, the cooling curves generated by terminating the power supply are not, at this time, an acceptable alternative method for calculating insulation.

DISCLAIMER

The views, opinions and/or findings in this report are those of the authors, and should not be construed as official Department of the Army position, policy or decision, unless so designated by other official documentation.

REFERENCES

1. Santee, WR., Chang, S. Kw. and Gonzalez, RR., Biophysical model for handwear insulation testing, *Aviat. Space Environ. Med.* 61: 481, 1990.
2. Einäs, S. and L. Holmér, Thermal insulation of handwear measured with an electrically heated hand model. In *Proceedings 1983: Int. Conf. on Protective Clothing Systems*, edited by K. Amundin, C. Brunius and A. Bränd-Persson, Stockholm, National Defense Research Institute, 1983.
3. Molnar, G.W., Heat transfer through the hand. In: *Protection and functioning of the hands in cold climates*, edited by F.R. Fisher, Washington, DC, National Academy of Science.